




ARM BATH

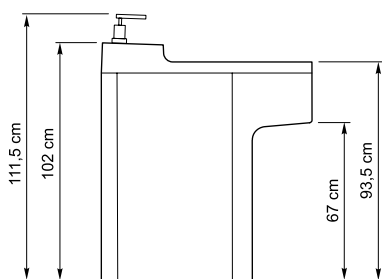


MEASURES FOR COMMUNICATIONS

- Drain for mud Ø 100 mm
- Drain for water Ø 50 mm
- H Hot water (3/4" stopcock max. 16 cm high from the floor)
- C Cold water (3/4" stopcock max. 16 cm high from the floor)
- ◇ Supply wire cable (1 m long)
- ⚡ Additional earthing wire cable (1 m long)
- M Mineral water (3/4" stopcock max. 16 cm high from the floor)

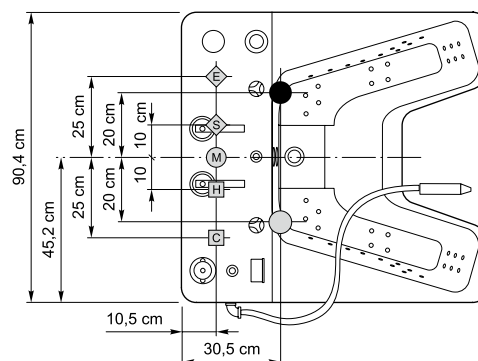

**HYDRO-USM-UVM
HYDRO-USM**


- Hydromassage
- Underwater shower massage
- Underwater vacuum massage
(only in the case of HYDRO-USM-UVM)
- Bath



	HYDRO-USM-UVM	HYDRO-USM
Power (kW)	2,2	2,2
Current (A)	10,4	10,4
Voltage (V)	220	220
Frequency (Hz)	50	50
• Nano jets	48	48
Underwater shower massage	1	1
Underwater vacuum massage	1	-

HYDRO


- Hydromassage
- Bath



Power (kW)	1,1
Current (A)	5,2
Voltage (V)	220
Frequency (Hz)	50
• Nano jets	48
Underwater shower massage	-
Underwater vacuum massage	-

USM-UVM


- Underwater shower massage
- Underwater vacuum massage
(only in the case of USM-UVM)
- Bath



	USM-UVM	USM
Power (kW)	1,1	1,1
Current (A)	5,2	5,2
Voltage (V)	220	220
Frequency (Hz)	50	50
Nano jets	-	-
Underwater shower massage	1	1
Underwater vacuum massage	1	-

W-M


- Drain for mud
- Bath



Power (kW)	-
Current (A)	-
Voltage (V)	-
Frequency (Hz)	-
Nano jets	-
Underwater shower massage	-
Underwater vacuum massage	-

BATH

- Bathtub body
- Frame with adjustable feet
- 2 front and 2 side panels
- Drain for water
- Hot and cold water stopcock
- Mixer with handshower



Power (kW)	-
Current (A)	-
Voltage (V)	-
Frequency (Hz)	-
Nano jets	-
Underwater shower massage	-
Underwater vacuum massage	-

TECHNICAL DATA

1. WATER PRESSURE IN THE SYSTEM OF UNDERWATER SHOWER MESSAGE DEVICE

Nozzle 7 mm	0-0,135 MPa
Nozzle 9 mm	0-0,125 MPa
Nozzle 11 mm	0-0,115 MPa

2. TIME FOR FILLING THE BATH

In the case of water pressure in the supplying system about 0,35 MPa and hot and cold water connections 3/4" – approximately 30 seconds.

3. TIME FOR DRAINING THE BATH

In the case of sanitation opening in the floor with Ø 50 mm and sanitation magistral pipe under the floor with Ø 50 mm – approximately 30 seconds.

4. MEASURES FOR CONNECTIONS OF HOT AND COLD WATER – 3/4".

5. MEASURES FOR CONNECTIONS OF MINERAL-, SEA- AND IODINE-BROMINE WATER – 3/4".

6. MEASURE FOR WATER DRAIN CONNECTION – outside Ø 50 mm.

7. MEASURE FOR MUD DRAIN CONNECTION – outside Ø 100 mm.